



**WISCONSIN STATE
LABORATORY OF HYGIENE**

Environmental Health Division
2601 Agriculture Drive
P.O. Box 7996
Madison, WI 53707-7996
Phone: (608) 224-6252 · (800) 442-4618
FAX: (608) 224-6213

University of Wisconsin

**National Filter Paper Blood Lead PT Program
July 2009 Testing Event**





August 06, 2009

Dear Participant:

Your individual performance report and statistical summary for the monthly Filter Paper Blood lead proficiency testing event are attached.

As always, please contact us with any questions you might have.


Sincerely,

Noel Stanton
Pb/EPPT Program Supervisor

Pb/EPPT Program, Toxicology Section
State Laboratory of Hygiene
2601 Agriculture Drive
Madison WI 53718

(608) 224-6252
toxpt@mail.slh.wisc.edu



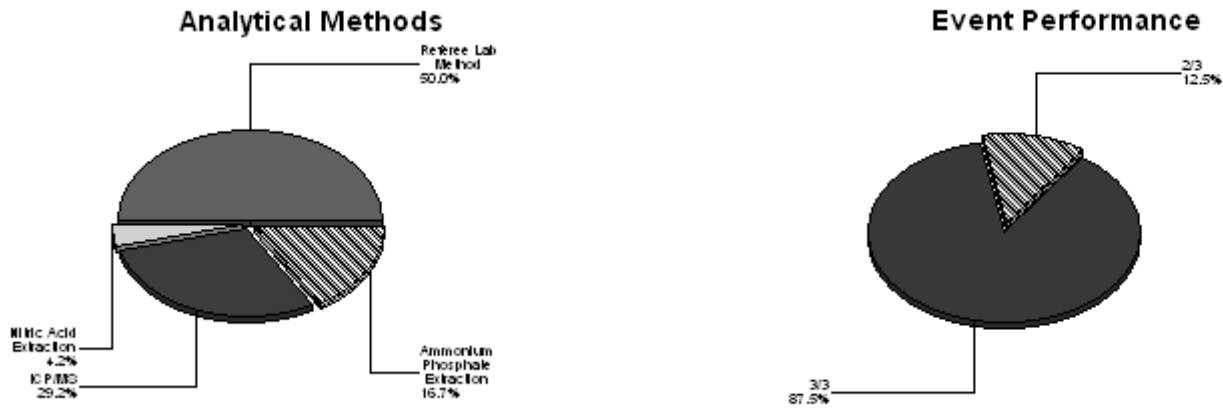

Target and Acceptable Range Information, ug/dL

Group	09FP23	09FP24	09FP25
Refereed Methods			
Target Value	28	18	1
Accepted Result	24-32	14-22	0-5

Method Statistics

Refereed Group	09FP23	09FP24	09FP25
Referee Laboratories (N=12)			
Mean	28.4	17.5	1.2
Standard Deviation	1.4	1.2	0.7
Number of Results *	12	12	12
All Laboratories (N=12)			
Mean*	27.8	17.8	1.1
Standard Deviation*	2.2	1.9	0.7
Participant Results (%Pass)	96	96	100
Ammonium Phosphate Extraction/GFAA (N=4)			
Mean*	28.0	19.0	0.8
Standard Deviation*	2.8	2.7	0.5
Participant Results (%Pass)	100	100	100
Nitric Acid Extraction/GFAA (N=1)			
Mean*	26.0	18.0	2.0
Standard Deviation*	0.0	0.0	0.0
Participant Results (%Pass)	100	100	100
ICP/MS (N=7)			
Mean*	27.0	17.4	2.7
Standard Deviation*	3.2	2.6	3.4
Participant Results (%Pass)	86	86	86

* Statistical outliers and alpha-numeric results (e.g. <X) have been excluded from the calculations

† Lack of statistical group consensus; all results deemed acceptable.

